

School of Chemistry Mass Spectrometry Service

SampleID CONEA
Sample Description
Analysis Name CONEA_254266_BD6_01_51481.d
Method 3a_AccMass_Loop_Positive.m
Instrument maXis impact

Source Type ESI **Ion Polarity** Positive

Submitter

Izar Capel

Supervisor


Malcolm Halcrow


Acquisition Date

29/11/2018 21:07:25

Scan Begin 50 m/z

Scan End 1500 m/z

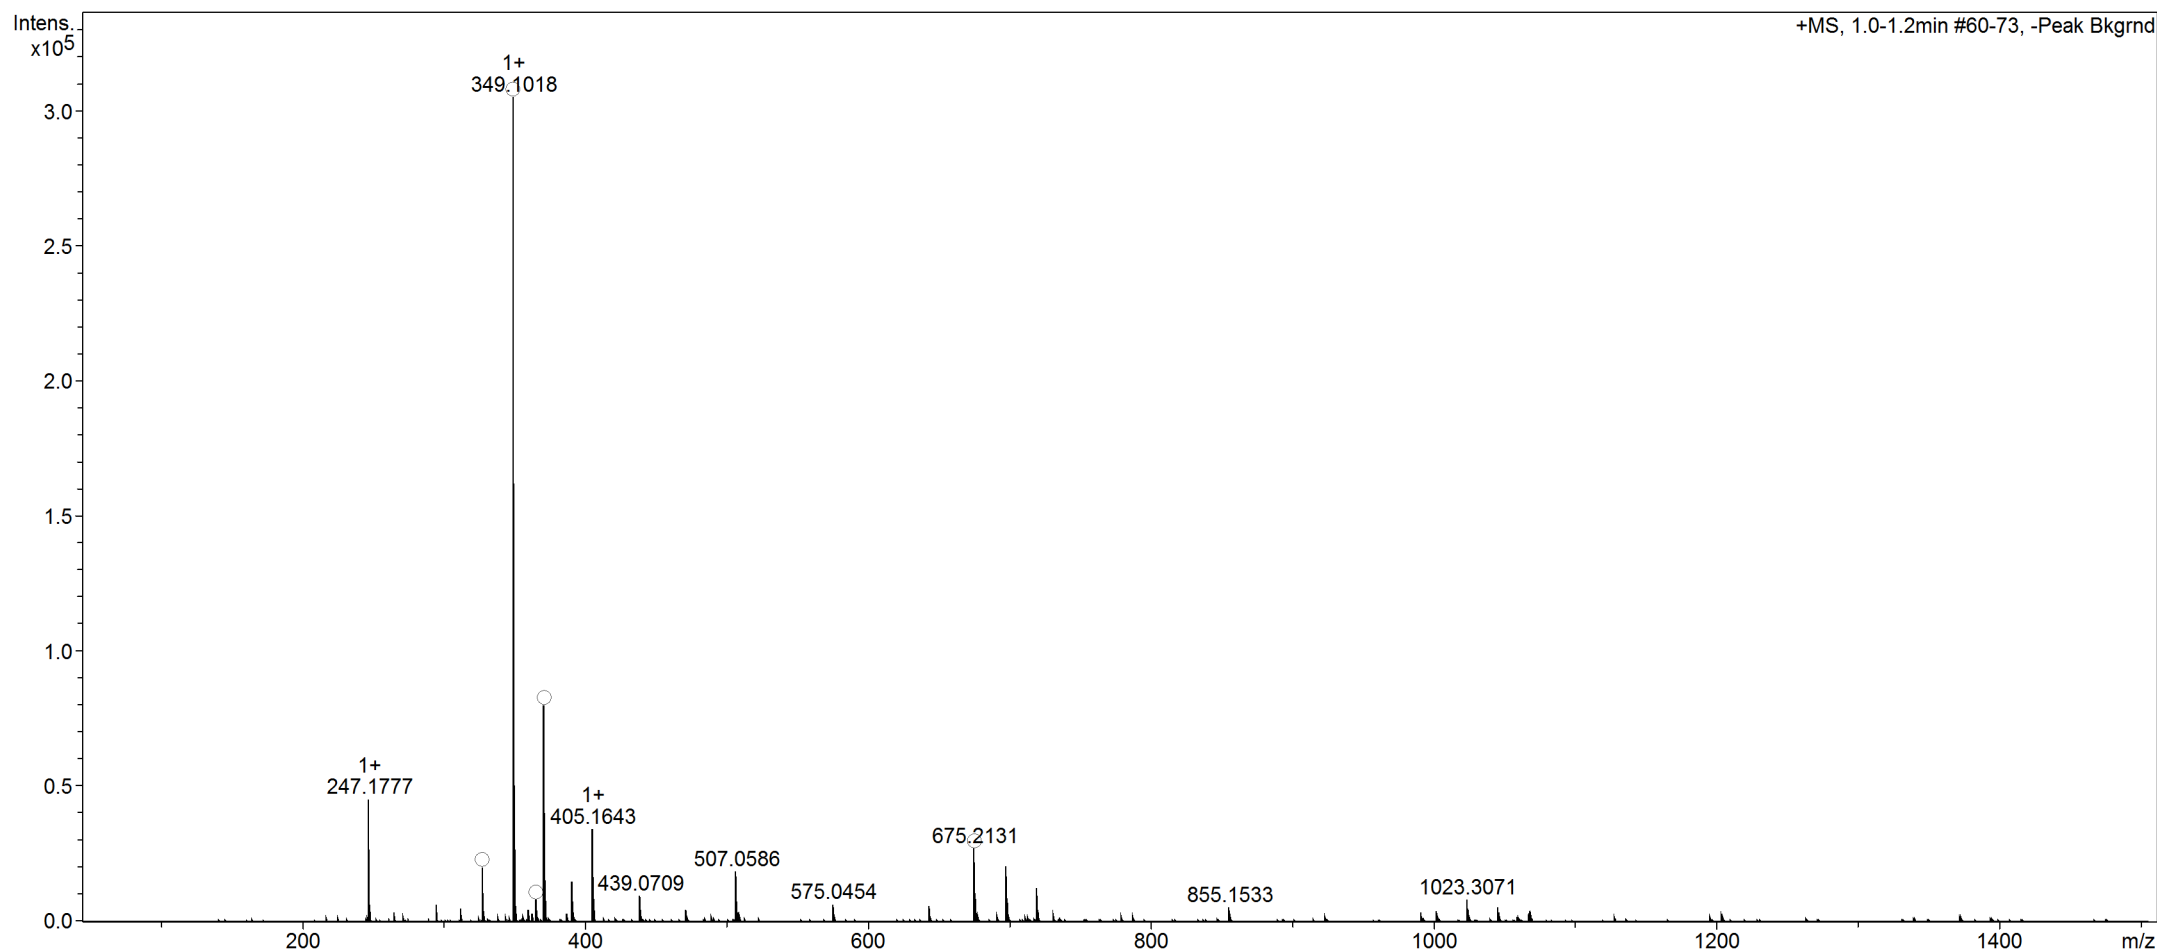

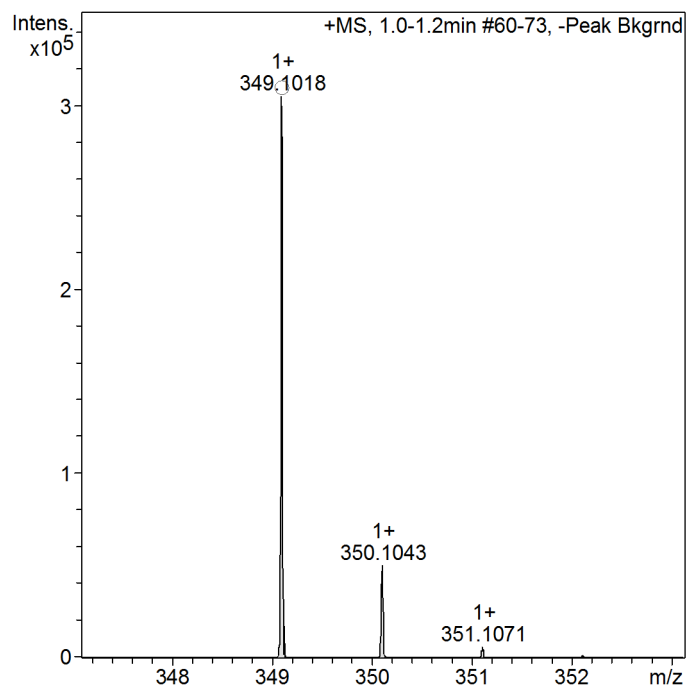

Confirm/Find Formula Results

The section below shows the results of formula calculation. If an expected formula was provided and found these are the results that are listed. If no formula was provided or no matches were found the system has attempted to determine the formula constrained by the parameters listed to the left

Meas. m/z	Ion Formula	z	m/z	err [mDa]	err [ppm]	mSigma	Score	Sum Formula	Adduct
327.120299	C15H15N6O3	1+	327.120015	-0.3	-0.9	10.3	100.00	C15H14N6O3	M+H
349.101829	C15H14N6NaO3	1+	349.101959	0.1	0.4	13.0	100.00		M+Na
365.075646	C15H14KN6O3	1+	365.075896	0.3	0.7	12.5	100.00		M+K
371.083759	C15H13N6Na2O3	1+	371.083903	0.1	0.4	4.2	100.00		M+Na2-H
675.213137	C30H28N12NaO6	1+	675.214697	1.6	2.3	10.2	100.00		2M+Na

Smart Formula Parameter	Value
Expected Formula	C15H14N6O3
Adducts Considered	

Smart Formula Search Parameters
CHNO and adducts considered implicitly

Formula Search Minimum
Formula Search Maximum

Algorithm Parameters	
Tolerance	4 ppm
Match to Isotope Pattern(mSigma)	40
Electron Configuration	even
Estimate No of Carbons	yes
Filter by H/C Ratio	0 < H/C < 3
Number of Double Bonds & Rings	0 < rings&DB < 80